

LCGreen® Plus+

Gene Scanning Reagent

Information Sheet

“The only dye for high-throughput, Hi-Res Melting™ analysis.”



Our new LCGreen PLUS is manufactured exclusively by Idaho Technology and is designed specifically for high resolution melting curve analysis to detect DNA sequence variants (SNP's, insertions / deletions).

Product Information

- LCGreen dyes are specifically designed for high-resolution melting curve analysis to detect DNA sequence variants (mutations, polymorphisms, etc).
- LCGreen PLUS is a new member of the dye family tailored for use in melting instruments with 96- or 384-well microtiter plates.
- LCGreen PLUS has superb fluorescence intensity, and can be used with other fluorescence based PCR detection systems such as the Roche LightCycler®. For optimal performance, the use of a high-resolution melting instrument is required.
- Optimum excitation: 440 – 470 nm. Optimum emission: 470 – 520 nm. Spectral characteristics depend on buffer composition, pH, ionic strength, and nucleic acid content of the solution.
- Addition of LCGreen dyes increase the melting temperature (T_m) of DNA by about 1 – 3 °C, and may require adjustment of cycling parameters.
- LCGreen dyes are manufactured exclusively by Idaho Technology, and their chemical structures are unique among the scientific and patent literature. Patent pending.

How it is Used

- LCGreen PLUS dye is supplied as a 10X solution in 10mM Tris-HCl, pH 7.4, 0.1 mM EDTA.
- LCGreen PLUS should be **used at 1X** for PCR. Add one volume of 10X solution to nine volumes of the PCR mixture.
- If you are using glass capillary tubes for PCR and/or for melting analysis, make sure your reaction mixture contains bovine serum albumin (BSA) at 250 - 500 µg/mL. BSA helps avoid enzyme, DNA and dye adhesion to the glass surface.


Shipping & Storage

- Product is shipped at ambient temperature.
- Store at –20 °C upon receipt. Store at 4 °C after first use.
- Product is stable for one year at –20 °C, and up to 2 months at 4 °C.

Related Products

- LightScanner™ (96 or 384 samples, high-resolution melting instrument)
- HR-1™ (single sample, high-resolution melting instrument)
- LCGreen® I gene scanning reagents (for use with Idaho Technology's HR-1)
- 10X BSA

Conventional dsDNA dyes cannot be used at high concentrations due to dye redistribution during melting curve analysis.

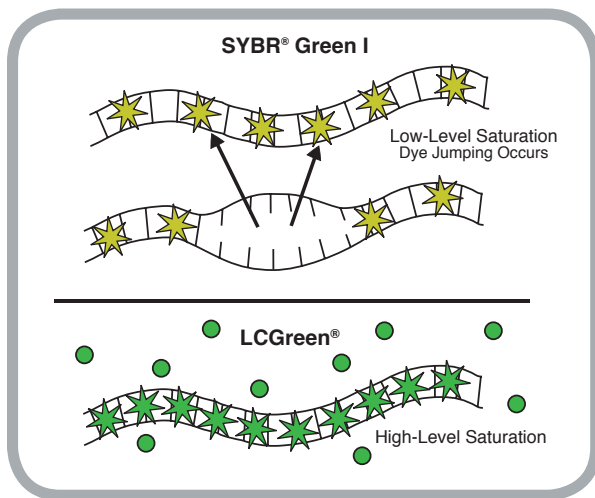

Saturation of dsDNA binding sites eliminates potential for dye redistribution during melting curve acquisition.

Package Sizes

No. of Reactions*	1,000	10,000	Larger sizes Inquire
LCGreen PLUS (10X solution)	1 mL	10 X 1 mL	
Catalog No.	BCHM-ASY-0005	BCHM-ASY-0006	

* based on 10 µl reaction volume


LCGreen, HR-1, LightScanner are trademarks of Idaho Technology Inc. LightCycler is a trademark of a member of the Roche Group. SYBR is a trademark of Molecular Probes.

References

1. Wittwer CT, GH Reed, CN Gundry, JG Vandersteen, and RJ Pryor. **High-Resolution Genotyping by Amplicon Melting Analysis using LC Green.** Clin. Chem., 49:853-60, 2003.
2. Liew M, Pryor R, Palais R, Meadows C, Erali M, Lyon E, Wittwer CT. **Genotyping of single nucleotide polymorphisms by high-resolution melting of small amplicons.** Clin. Chem., 50:1156-64, 2004.
3. Reed GH, Wittwer CT. **Sensitivity and specificity of SNP scanning by high-resolution melting analysis.** Clin. Chem., 50:1748-54, 2004.
4. Zhou L, Myers AN, Vandersteen JG, Wang L, Wittwer CT. **Closed-Tube Genotyping with Unlabeled Oligonucleotide Probes and a Saturating DNA Dye.** Clin Chem., 50:1328-35, 2004
5. McKinney JT, Longo N, Hahn SH, Matern D, Rinaldo P, Strauss AW, Dobrowolski SF. **Rapid, comprehensive screening of the human medium chain acyl-CoA dehydrogenase gene.** Mol Genet Metab. 82:112-20, 2004.
6. Willmore BS, Holden JA, Zhou L, Tripp S, Wittwer CT, Layfield LJ. **Detection of c-kit activating mutations in gastrointestinal stromal tumors by high-resolution amplicon melting analysis.** Am. J. Clin. Path., 122:206-16, 2004.
7. Zhou L Vandersteen J, Wang L, Fuller T, Taylor M, Palais B, Wittwer CT. **High-resolution DNA melting curve analysis to establish HLA genotypic identity.** Tissue Antigens, 64:156-64, 2004.
8. Vaughn CP, Elenitoba-Johnson KS. **High-resolution melting analysis for detection of internal tandem duplications.** J. Mol. Diag. 6:211-6, 2004.
9. Odell ID, Cloud JL Seipp M, and Wittwer CT. **Rapid species identification within the Mycobacterium chelonae-abscessus group by high-resolution melting of hsp65 PCR products.** Am J Clin Path 2005;123:96-101.
10. Dobrowolski SF, McKinney JT, Amat di San Filippo C, Giak Sim K, Wilcken B, Longo N. **Validation of dye-binding/high-resolution thermal denaturation for the identification of mutations in the SLC22A5 gene.** Hum Mutat. 2005 Mar;25(3):306-13

Reviews on High-Resolution Melting

1. Gingeras TR, Higuchi R, Kricka LJ, Lo YM, Wittwer CT. **Fifty Years of Molecular (DNA/RNA) Diagnostics.** Clin Chem., 51:661-71, 2005
2. Highsmith WE Jr., **SNPs for sale. Cheap!.** Clin Chem., 50:1296-8, 2004

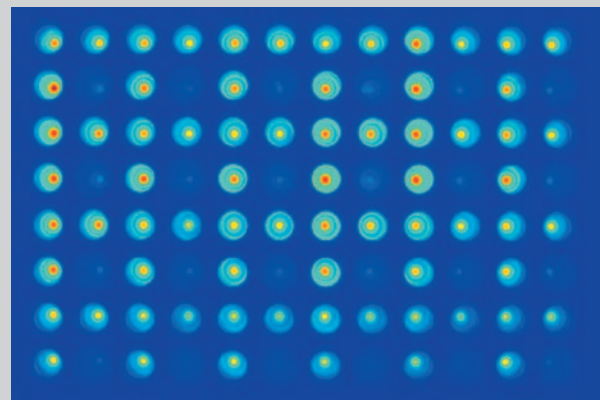

DNA visualized with LCGreen PLUS dye in a 96-well plate with Idaho Technology's LightScanner™ instrument.